

Burette, Digital, Solar Powered, Conformity certified, with Individual Work Certificate, High Precision Digital Titrator for exact and error - free Titration, SOLARUS. The unit will be supplied complete with mounted discharge unit and A45 female thread. 3 different adapters (A 32, A 30 & A 40), suction tube, return tube and wrench



Cat No.	Capacity ml	Accuracy R ≤ ± %	Reproducibility CV ≤ %	Qty. Per Pack Pcs
93920 10	10	0.3	0.1	1
93920 20	20	0.2	0.1	1
93920 50	50	0.2	0.1	1

LABOPETTE, Fixed Volume, Conformity Certified with Individual Work Certificate, HIRSCHMANN

Cat No.	Capacity ml	Accuracy R ≤ ± %	Reproducibility CV ≤ %	Qty. Per Pack Pcs
94755 01	5	2.5	1.5	1
94755 02	10	1.2	0.8	1
94755 03	20	1.0	0.5	1
94755 04	25	1.0	0.5	1
94755 05	50	1.0	0.4	1
94755 06	100	0.8	0.3	1
94755 07	200	0.8	0.3	1
94755 08	250	0.8	0.3	1
94755 09	500	0.8	0.3	1
94755 10	1000	0.8	0.3	1
94755 11	2000	0.8	0.3	1
94755 12	5000	0.8	0.3	1
94755 13	10 ml	0.6	0.3	1



LABOPETTE, Variable Volume, Conformity Certified with Individual Work Certificate, HIRSCHMANN

Cat No.	Volume µl	Volume Division µl	Accuracy R ≤ ± %	Reproducibility CV ≤ %	Qty. Per Pack Pcs
94754 00	0.1 - 3	0.002	4.0	2.0	1
94754 01	0.5 - 10	0.01	1.2	0.8	1
94754 06	2 - 20	0.02	1.0	0.5	1
94754 07	10 - 100	0.1	0.8	0.3	1
94754 08	20 - 200	0.2	0.8	0.3	1
94754 09	100 - 1000	1.0	0.8	0.3	1
94754 05	500 - 5000	10.0	0.8	0.3	1
94754 04	1 - 10 ml	20.0	0.6	0.3	1

LABOPETTE, Variable Volume, Multi Channel, Conformity Certified with Individual Work Certificate, HIRSCHMANN

Cat No.	No. of Channels	Volume µl	Volume Division µl	Accuracy R ≤ ± %	Reproducibility CV ≤ %	Qty. Per Pack Pcs
94756 01	8	0.5 - 10	0.01	2.4	1.6	1
94756 02	8	10 - 100	0.1	1.6	0.6	1
94756 04	8	30 - 300	0.2	1.6	0.6	1
94757 01	12	0.5 - 10	0.01	2.4	1.6	1
94757 02	12	10 - 100	0.1	1.6	0.6	1
94757 04	12	30 - 300	0.2	1.6	0.6	1




PIPETUS - Pipetting Device for All Conventional Glass Pipettes, HIRSCHMANN

Cat No.	Equipment Type	Operating Principle	Operating Range ml	Accessories Supplied	Qty. Per Pack Pcs
99020 00	Junior	Manual	0.5 - 10		1
99030 00	Standard	Electrical	0.1 - 100	Elect. Pump	1
99072 00	Akku	Electrical	0.1 - 100	Bat. Charger	1






Pipette Stand

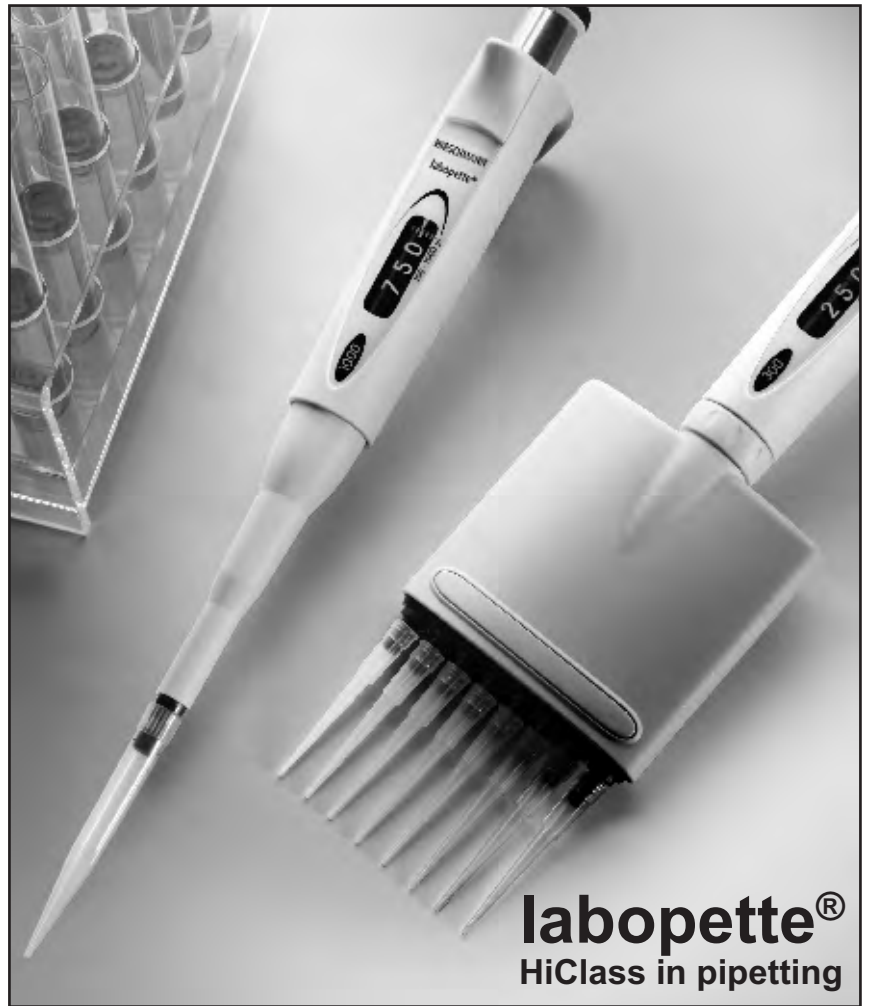

labopette®
HiClass in pipetting

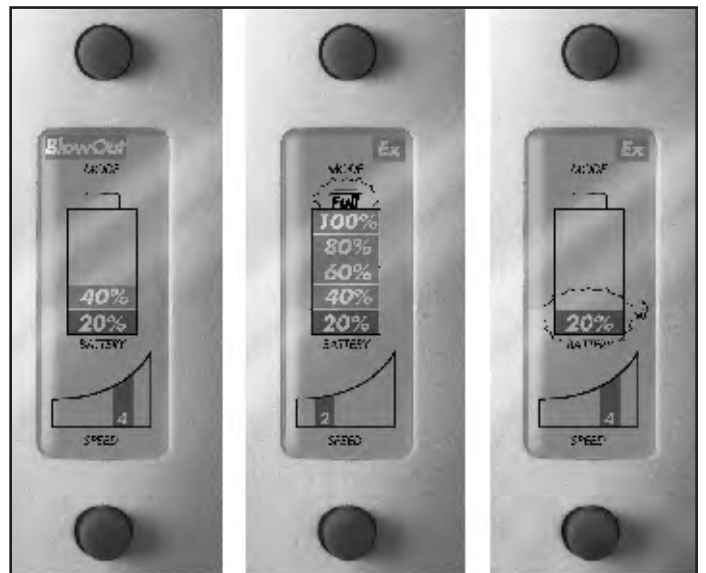

pipetus® standard



pipetus® junior